SmartGuard

User Guide

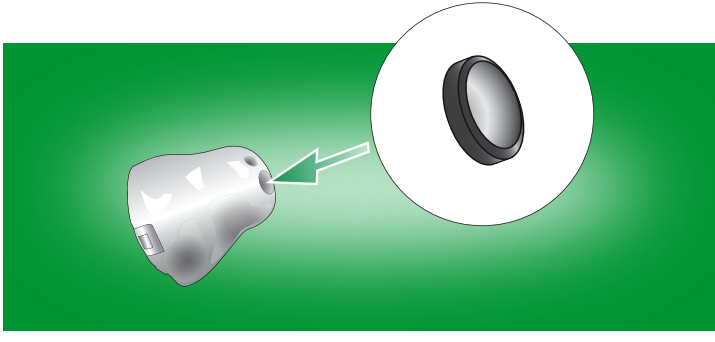

PHONAK
hearing systems

CE

Welcome

SmartGuard from Phonak provides the most advanced wax protection technology available and significantly increases the lifetime of your hearing system.

SmartGuard unites breakthrough technology with simple, easy to use tools - the ultimate solution for reliable protection against long-term damage due to wax and moisture.

Please read this brochure carefully to learn how to obtain the maximum benefit from your SmartGuard wax protection system. Following these guidelines will optimize the SmartGuard system and will ensure optimal performance from your hearing instrument.

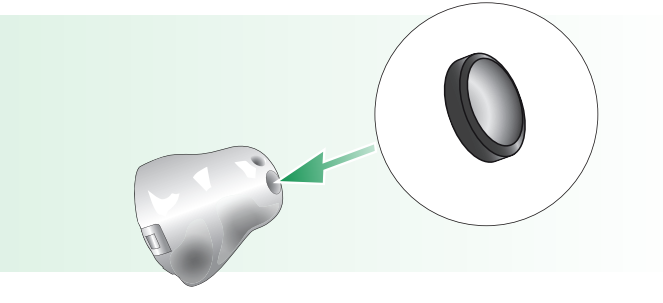

Cleaning your SmartGuard

Clean SmartGuard daily by simply wiping with a soft cloth or tissue. Do not apply excessive pressure to the tip of the hearing instrument.

① Use a gentle back and forth wiping motion.
② Never wipe with a rotating motion as this might damage the SmartGuard.
③ Never use water to clean the SmartGuard.
④ Never use sharp objects or brushes to clean the SmartGuard.

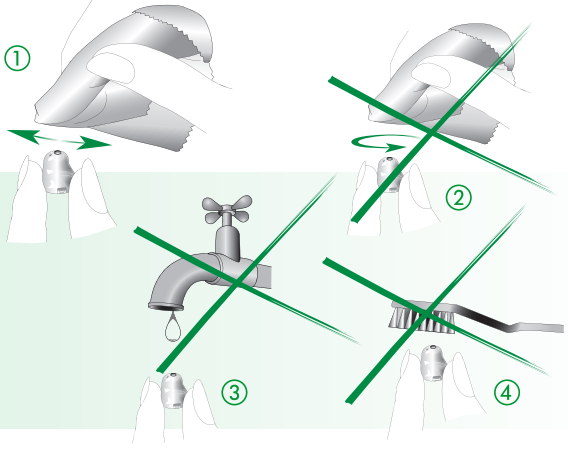

Changing your SmartGuard

- For best results change your SmartGuard every two months or as recommended by your hearing care professional.
- Use only the supplied handling tool when changing the SmartGuard.
- SmartGuards and handling tools are designed for single use only. Please dispose after use.

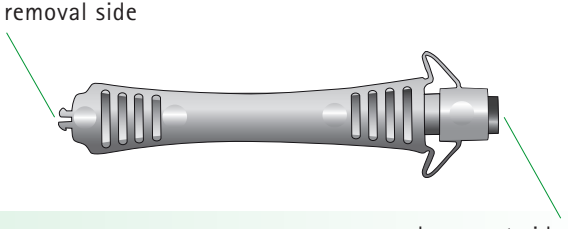

Removal of the used SmartGuard

① Gently press the removal side of the tool into the SmartGuard ring until you feel the tool snap in.
② The SmartGuard ring will be attached to the tool as you gently pull the tool back.
③ Keep the tool straight as you remove the SmartGuard ring. This will help to maintain a firm grip on the used SmartGuard ring.

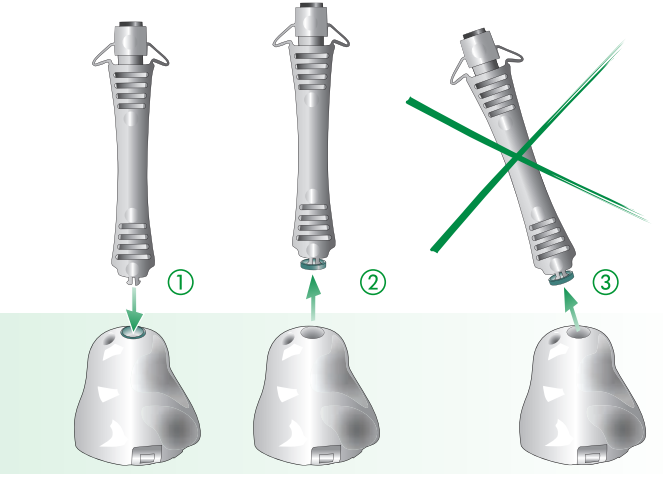

Insertion of a new SmartGuard

① A new SmartGuard ring is already attached to the replacement side of the handling tool.

② Place the replacement side against the sound outlet of the hearing instrument and press gently until you feel the SmartGuard snap into place.

③ Gently pull the tool back.
The hearing instrument is now ready for use.

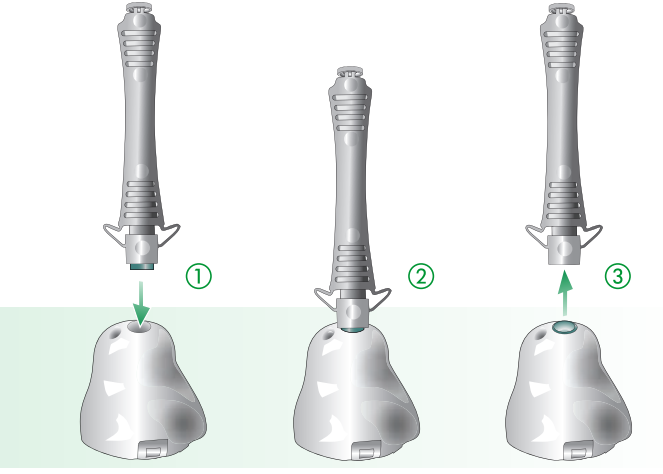

CE The CE symbol is confirmation by Phonak AG that this product meet the requirements of directive 93/42/EEC on medical devices.

Operating conditions

SmartGuard has been designed for trouble-free operation under all ordinary climatic conditions.

Transportation and storage conditions

Temperature should not exceed limits of –20°/60°Celsius at a relative air humidity of 65% for extended periods during transportation and storage. Air pressure between 500 and 1100 hPa is not detrimental to SmartGuard.

Not suitable for children under 3 years.

For single use only.